


SURVEYOR® Mutation Detection Kit Fluorescent Capillary Electrophoresis and PAGE

Discover and Detect All Types of Genetic Variations

SURVEYOR Mutation Detection Kits provide a simple, accurate and cost-effective means to scan DNA fragments for mutations with unmatched sensitivity and specificity.

Complete Mutation Detection System: Contains SURVEYOR Nuclease, all reagents and plasmid controls.

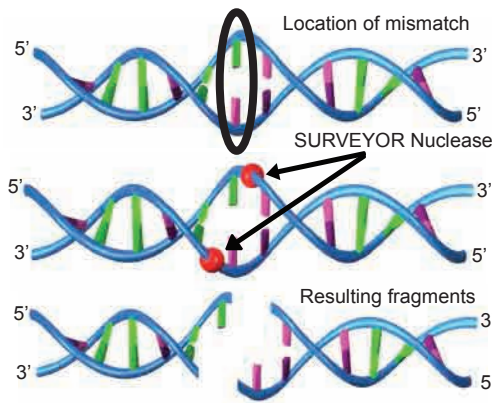


SURVEYOR Nuclease is a mismatch-specific endonuclease that recognizes mismatches in heteroduplexed DNA and cleaves both strands on the 3' side of the mismatch providing specific information on mutation location, orientation and type.

Designed for Multiple Mutation Discovery Applications

- Somatic, germ-line and mitochondrial mutations
- Insertions, deletions, substitutions and SNPs
- Low-copy mutations and pooled DNA samples


Mutation Detection in Four Easy Steps

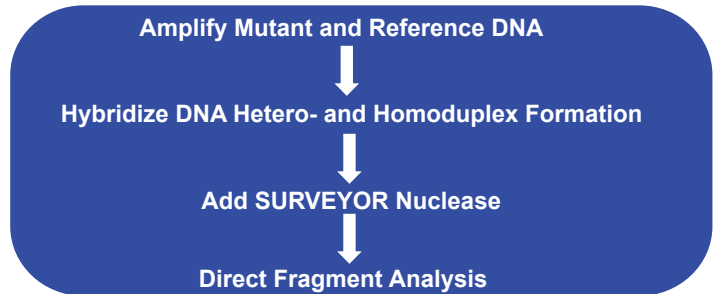

Benefits

- Determines mutation loci
- Saves time and money
 - Streamlines DNA sequencing
 - Decreases sequencing backlog and analysis time
 - Validates sequencing results and analysis
 - Decreases chromatogram analysis by 90%
- No post-PCR or post-reaction clean-up
- High throughput sensitivity and specificity

Figure 1. Capillary electrophoresis analysis of fragments generated by digestion of 160 ng of FAM end-labeled DNA with 1 µl of SURVEYOR Nuclease F at 42°C for 10 min. Analysis of one twentieth of the digested DNA was performed. The 584-bp amplicons were PCR amplified with Optimase Polymerase from one wild type and three mutant *E. coli lacZ* genes. The mutants had one (T>C), two (A>G and T>C), and three (1 base deletion, T>C and C>A) mutations. For each mutation, partial digestion with SURVEYOR Nuclease generated two detectable end-labeled fragments. Numbers (in base pairs) indicate the sizes of the FAM-labeled fragments and the full-length FAM-labeled homoduplex control (HMD). The DNA standard ladder was used to size the fragments.

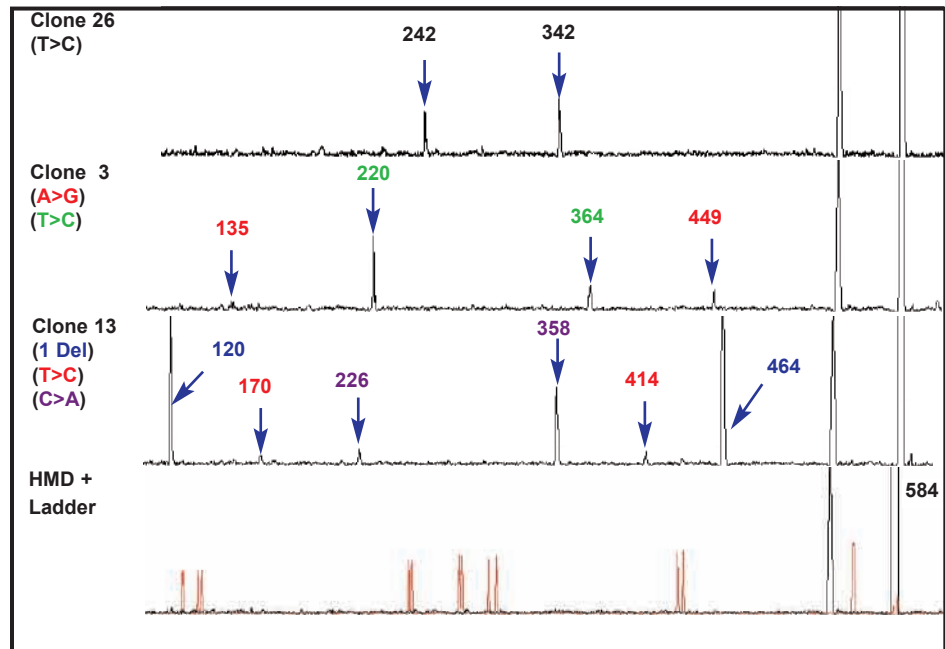

SURVEYOR Mutation Detection Kit Components – All Optimized to Work Together

- SURVEYOR Nuclease F
- SURVEYOR Nuclease Enhancer F
- Stop Solution
- Control Plasmids and Primers

Products

SURVEYOR Mutation Detection Kit for Fluorescent Capillary Electrophoresis and PAGE

Quantity	Catalog No.
25 reactions	706015
100 reactions	706010

SURVEYOR Nuclease can also be obtained in bulk, please call 1-240-631-2001 for more information.

Related Products

Mutation detection performance and sensitivity of the SURVEYOR Mutation Detection Kits are significantly enhanced by using a proofreading thermostable DNA polymerase for the PCR step. Optimase® Polymerase, available from Transgenomic, was used to develop the optimized protocols for these kits.

	Catalog No.	Quantity
Optimase Polymerase with dNTPs	SP2024	100 units

Shipping and Storage

SURVEYOR products are shipped frozen. Store product at -20° C in a non-frost-free freezer. Enzyme is guaranteed for a period of 6 months if stored as directed.

Quality Control

Every component has met Transgenomic quality control standards. Refer to the *Certificate of Analysis* for details.

Selected References

- 1. Rapid identification of unknown heteroplasmic mutations across the entire human mitochondrial genome with mismatch-specific Surveyor Nuclease** Bannwarth, S., Procaccio, V., Paquis-Flucklinger, V., *Nature Protocols* VOL.1, NO.4 2037-2047. (2006).
- 2. Allelic dilution obscures detection of a biologically significant resistance mutation in EGFR -amplified lung cancer.** Engelman, J.A., Mukohara, T., Zejnullahu, K., Lifshits, E., Borras, A.M., Gale, C.M., Naumov, G.N., Yeap, B.Y., Jarrell, E., Sun, J., Tracy, S., Zhao, X., Heymach, J.V., Johnson, B.E., Cantley, L.C., Janne, P.A., *J. Clin. Invest.* 116, 2695-2706. (2006).
- 3. The JAK2 V617F mutation occurs in hematopoietic stem cells in polycythemia vera and predisposes toward erythroid differentiation.** Jamieson, C.H., Gotlib, J., Durocher, J.A., Chao, M.P., Mariappan, M.R., Lay, M., Jones, C., Zehnder, J.L., Lilleberg, S.L., Weissman, I.L. *Proc. Natl. Acad. Sci.* 103, 6224-6229 (2006).
- 4. A rapid and sensitive enzymatic method for epidermal growth factor receptor mutation screening.** Janne, P.A., Borras, A.M., Kuang, Y., Rogers, A.M., Joshi, V.A., Liyanage, H., Lindeman, N., Lee, J.C., Halmos, B., Maher, E.A., Distel, R.J., Meyerson, M., Johnson, B.E. *Clin. Cancer Res.* 12, 751-758. (2006).
- 5. Temperature-mediated heteroduplex analysis for the detection of drug-resistant gene mutations in clinical isolates of Mycobacterium tuberculosis by denaturing HPLC, SURVEYOR nuclease.** Shi, R., Otomo, K., Yamada, H., Tatsumi, T., Sugawara, I. *Microbes Infect.* 8, 128-135. (2006).
- 6. A new detection method for ATRX gene mutations using a mismatch-specific endonuclease.** Wada, T., Fukushima, Y., Saitoh, S. *Am. J. Med. Genet. A* 140, 1519-1523. (2006).

Corporate Headquarters

Transgenomic, Inc.
12325 Emmet Street
Omaha, NE 68164, USA
Phone: (888) 233-9283 • (402) 452-5400
Fax: (402) 452-5401
Email: info@transgenomic.com

Transgenomic Limited
40 Watt Road, Hillington Park
Glasgow G52 4RY, UK
Phone: +44 (0) 141 892 8800
Fax: +44 (0) 141 883 5967
Email: sales@transgenomic.com



www.transgenomic.com

Document No. 602085-01
10/2008